

Retrospective Correction of Involuntary Microscopic Head Movement Using Highly Accelerated Fat Image Navigators (3D FatNavs) at 7T

Daniel Gallichan,^{1*} José P. Marques,² and Rolf Gruetter^{1,2,3}

Purpose: The goal of the present study was to use a three-dimensional (3D) gradient echo volume in combination with a fat-selective excitation as a 3D motion navigator (3D FatNav) for retrospective correction of microscopic head motion during high-resolution 3D structural scans of extended duration. The fat excitation leads to a 3D image that is itself sparse, allowing high parallel imaging acceleration factors – with the additional advantage of a minimal disturbance of the water signal used for the host sequence.

Methods: A 3D FatNav was inserted into two structural protocols: an inversion-prepared gradient echo at $0.33 \times 0.33 \times 1.00$ mm resolution and a turbo spin echo at $600 \mu\text{m}$ isotropic resolution.

Results: Motion estimation was possible with high precision, allowing retrospective motion correction to yield clear improvements in image quality, especially in the conspicuity of very small blood vessels.

Conclusion: The highly accelerated 3D FatNav allowed motion correction with noticeable improvements in image quality, even for head motion which was small compared with the voxel dimensions of the host sequence. **Magn Reson Med** 75:1030–1039, 2016. © 2015 Wiley Periodicals, Inc.

Key words: retrospective motion correction; navigators; FatNavs

INTRODUCTION

Recent technological developments in both hardware and software have led to substantially increased spatial resolution in MRI. As resolution improves, the image quality is increasingly sensitive to small involuntary motion of the subject. Various motion correction methods have been proposed, including techniques using external markers for a tracking system (1–5) or MR navi-

gator-based methods that can either use data directly from the imaging sequence itself (6,7) or interleave a rapid navigator within the host sequence (8–11). The majority of existing methods have concentrated on the correction of moderate- to large-scale motion of the subject (approximately >5 mm translation and approximately $>5^\circ$ rotation), with healthy volunteers being asked to make deliberate movements in order to test the correction methods. Recent work has also demonstrated the utility of the detection and correction of the microscopic motion of compliant subjects (root-mean-square approximately ≤ 2 mm translation and approximately $\leq 2^\circ$ rotation) that is unavoidable for durations required for imaging at very high spatial resolution (3,5,12). An external camera/marker system was used to achieve these results, for which the spatial constraints of the MR system and radiofrequency (RF) head coil can cause installation difficulties. Modern MR systems often have RF arrays for neuroimaging with ≥ 32 receive channels and close-fitting designs that leave little room to establish a line of sight between a bore-mounted camera and markers attached to the subject's head. An existing approach that is compatible with most RF coil designs is to mount the marker on a dental-fit mouthpiece (5,12); however, this approach must be customized for each subject, limiting how readily the method may be applied for routine use.

A recent preliminary study demonstrated that very high-resolution images ($350 \mu\text{m}$ isotropic) could be achieved at 3T using a 138-min protocol interleaved with volumetric echo planar imaging (EPI)-based navigators (vNavs) (13). It is unclear, however, what the expected precision of the vNavs should be in their current implementation (8 mm isotropic resolution multi-shot EPI), and it is expected that this performance would diminish at 7T because of the increased image distortions and signal dropouts due to increased B_0 variations at higher fields.

It has been demonstrated previously that a fat-selective RF pulse can be useful as a motion navigator for cardiac applications (14), and some studies have also been performed for head imaging (15). Therefore, the aim of the present study was to demonstrate the feasibility of a navigator-based correction method at 7T suitable for high-resolution imaging with no deliberate motion of the subject and requiring a negligible increase in scan time, exploiting the natural sparsity of fat-only head images (as the signal is primarily localized to sub-cutaneous fat and bone-marrow in the skull) to allow a highly accelerated parallel acquisition. It has been noted in other

¹Centre d'Imagerie BioMédicale (CIBM), EPFL Lausanne, Lausanne, Switzerland.

²Department of Radiology, University of Lausanne, Lausanne, Switzerland.

³Department of Radiology, University of Geneva, Geneva, Switzerland

Grant sponsor: Centre d'Imagerie BioMédicale (CIBM) of the UNIL, UNIGE, HUG, CHUV, EPFL and the Leenaards and Jeantet Foundations; Grant sponsor: Swiss National Science Foundation; Project number: 205321_153564.

*Correspondence to: Daniel Gallichan, D.Phil., CIBM, EPFL-SB IPSB LIFMET, Station 6, CH-1015 Lausanne, Switzerland. E-mail: daniel.gallichan@epfl.ch


Presented in abstract form at the 22nd Annual Meeting of the International Society of Magnetic Resonance in Medicine, Milan, Italy, 2014.

Received 8 August 2014; revised 12 January 2015; accepted 31 January 2015

DOI 10.1002/mrm.25670

Published online 14 April 2015 in Wiley Online Library (wileyonlinelibrary.com).

FIG. 1. Pulse sequence diagrams of (a) the MP2RAGE sequence and (b) the TSE sequence as used in Experiments 3 and 4, showing the relative timing of the 1152 ms 3D FatNav (isotropic resolution, 2 mm; acceleration, 4×4).

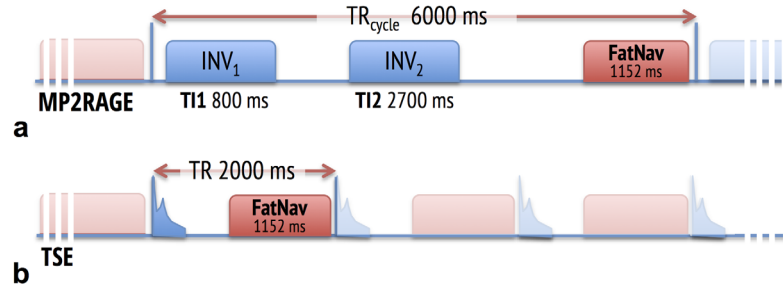

recent work on fat-based navigators (16) that acceleration factors of up to 8 could be used for a two-dimensional fat image with only minor image degradation, using a conventional generalized autocalibrating partially parallel acquisitions (GRAPPA) method (17) for image reconstruction on data acquired with an eight-channel RF coil. In our study we used a 32-channel coil and a 3D acquisition, allowing even higher acceleration factor.

METHODS

All imaging was performed on a 7T head-only MR system (Siemens Healthcare, Erlangen, Germany) fitted with a 32-channel RF coil array, housed within a birdcage transmit coil (Nova Medical Inc., Wilmington, Massachusetts, USA). All volunteers were healthy young adults (19–35 years) who provided written informed consent prior to the imaging in accordance with the local review board.

Highly Accelerated Fat Motion Navigators

With the aim of correcting for microscopic level motion, we chose an isotropic resolution of 2 mm for the highly accelerated fat motion navigators (3D FatNavs) with the expectation that this will be approximately sufficient to detect motion at a level similar to that reported for a ballisto-cardiogram of $\sim 140 \mu\text{m}$ (5)—motion that occurs very quickly during the cardiac cycle and represents an upper limit on the useful resolution of a navigator that will not be fast enough to track this small motion. A 3D gradient echo (GRE) acquisition was used with a three-pulse binomial excitation pulse to selectively excite at the frequency of fat (~ 1000 Hz from water at 7T) using the following parameters: matrix size = $88 \times 128 \times 128$; echo time (TE)/repetition time (TR) = 1.35/3.0 ms; bandwidth = 1950 Hz/pixel; flip angle = 7° ; and a foot/head readout direction. Partial Fourier undersampling (reconstructed with zero-filling) was used for all FatNavs to reduce the $\text{TR}_{\text{volume}}$ by 44% at the expense of a small loss of effective resolution. A fully sampled acquisition with these parameters requires 19.0 s.

Experiment 1: Evaluation of Achievable GRAPPA Acceleration for 3D FatNavs

Two fully sampled volumes were acquired with the parameters described above. After a Fourier transform in the readout direction, a single transverse slice of data was selected as an example for testing acceleration factors. The central 20×32 samples from the first volume

were used for the calibration of the GRAPPA weights. The data from the second volume were decimated to simulate various acceleration factors (2 to 10 per phase-encoding direction, corresponding to total acceleration of 4–100 times), and then reconstructed using a GRAPPA kernel with 2×2 source points at each acceleration factor. The same process was repeated with a nonselective excitation to compare the reconstruction quality at each acceleration factor with a conventional water image.

Experiment 2: High-Resolution MP2RAGE Scan Motion-Corrected with 3D FatNavs

An acceleration factor of $4 \times 4 = 16$ was chosen for the 3D FatNav used to correct the structural data, as the results of Experiment 1 indicated a good image quality at this acceleration factor, and the navigator duration of 1.15 s can be inserted into existing high-resolution protocols for MP2RAGE (magnetization prepared 2 rapid acquisition gradient echoes [18]) acquisitions without additional scan time, as there is already sufficient “dead time” between inversion pulses waiting for signal recovery. The binomial pulse used for fat excitation has a low flip angle (7°) for fat and is therefore expected to have a negligible effect on the water signal recovery, despite 384 excitations during the 1.15 s.

For the MP2RAGE scan, a nominal resolution of $0.33 \times 0.33 \times 1.00$ mm was used (matrix size = $488 \times 492 \times 80$; field of view = $160 \times 160 \times 80$ mm; 6/8 partial Fourier), which allowed coverage of most of the brain, using the following parameters: TE/inversion time (TI_1/TI_2)/TR = 6.06/800/2700/6000 ms; bandwidth = 280 Hz/pixel; flip angle (TI_1/TI_2) = $7^\circ/5^\circ$; anterior/posterior readout direction; right/left phase-encoding direction; and flow compensation in the partition-encoding direction. The total scan time for the MP2RAGE scan was 36 min, 38 s, and an additional 2.3 s was added to the start of the scan to acquire 20×32 lines of fully sampled fat excitation data from which to determine the GRAPPA weights for the 3D FatNavs using a 2×2 kernel. Figure 1a shows a diagram of one TR of the pulse sequence and the relative timing of the 3D FatNav.

All raw data were processed using MATLAB (MathWorks, Natick, Massachusetts, USA). We first reconstructed each of the 366 3D FatNavs, then performed rigid body coregistration of each 3D FatNav to the first using a least-squares cost function with the *realign* tool in SPM (Statistical Parametric Mapping, version 8) using the highest “quality” setting (1.0) and with the other parameters left at their default settings (5 mm full-width

half-maximum Gaussian smoothing prior to realignment, degree 2 B-spline interpolation, 4 mm separation of image samples). The estimated motion parameters were subsequently recentered such that “zero motion” was defined as the time coincident with the acquisition of the center of k-space (1/3 of the total scan time due to use of partial Fourier undersampling) in order to maintain the strongest visual similarity between reconstructed images before and after motion correction. Retrospective motion correction of the MP2RAGE data was performed in k-space using the motion parameters from the 3D FatNav acquired closest in time (effectively applying one set of motion parameters per k-space plane in the partition-encoding direction), with translations corresponding to simple phase ramps, and rotations requiring 3D regridding, which was performed using the 3D non-uniform fast Fourier transform algorithm (19) provided by Jeffrey Fessler’s reconstruction toolbox (<http://web.eecs.umich.edu/~fessler/code/>). Assuming small motion, no density compensation was applied to compensate for the changes in k-space sample density resulting from the rotations. All corrections were performed separately for the data from each RF channel prior to calculating the MP2RAGE image by combination of the complex images from each inversion time:

$$\text{MP2RAGE}_\alpha = \text{real} \left(\frac{\text{GRE}_{\text{TI1},\alpha}^* \text{GRE}_{\text{TI2},\alpha}}{|\text{GRE}_{\text{TI1},\alpha}|^2 + |\text{GRE}_{\text{TI2},\alpha}|^2} \right) \quad [1]$$

where $\text{GRE}_{\text{TI1},\alpha}$ is the image generated from the data acquired at the first inversion time (TI1) for the coil channel index α , and the asterisk denotes complex conjugation. The final MP2RAGE image was combined from each coil channel as a weighted sum, where the weight was determined by $|\text{GRE}_{\text{TI2},\alpha}|^2 / \sum_i |\text{GRE}_{\text{TI2},i}|^2$ for each voxel in each coil. The (unoptimized) regridding process took ~ 5 min per volume per RF channel on a Linux server with a 2×8 core 2.66 GHz CPUs and 96 GB of RAM.

It has previously been noted that inversion-prepared GRE sequences can also be used for vessel visualization (20). The coil-combined image from the second inversion time, GRE_{TI2} , which was used to demonstrate vessel contrast, was produced by a root sum-of-squares from the separate coil images. The resulting GRE_{TI2} image was then processed using FAST software (FMRIB’s Automated Segmentation Tool (21), part of the FMRIB Software Library, version 5.0) to allow “bias-field” correction to reduce the signal intensity variations across the brain due to the spatially varying sensitivity of the RF array. A projection of the maximum intensity over a thick slab allows visualization of arteries, and a minimum intensity projection allows visualization of veins.

Experiment 3: High-Resolution Turbo Spin Echo Scan Motion-Corrected with 3D FatNavs

For the turbo spin echo (TSE) sequence, a different volunteer was scanned with nominal isotropic resolution of 600 μm (matrix size = $384 \times 384 \times 288$; field of view = $230 \times 230 \times 172.8$ mm; 6/8 partial Fourier undersampling in the partition-encoding direction. TE/

TR = 119/2000 ms, bandwidth = 543 Hz/pixel, turbo factor 110, echo train duration 362 ms, readout direction foot/head, phase-encoding direction anterior/posterior, variable flip angle train using vendor-supplied implementation based on the scheme described in Mugler et al. (22). The total scan time was 33 min 56 s, with an additional 2.3 s for the GRAPPA calibration data for the 3D FatNavs. Figure 1b shows the relative timing of the pulse sequence and the inclusion of the 3D FatNav.

Experiment 4: Detection of Head-Motion Due to the Respiratory Cycle with FatNavs

It has been demonstrated previously with external motion-tracking hardware that there is typically a small head motion associated with the cardiac and respiratory cycles while a subject is lying supine within the MR system, predominantly along the z-axis (3,5). As preliminary experiments suggested that the precision of motion-estimation using the current parameters for the 3D FatNavs should be sufficient to detect motion on this order (approximately $<100 \mu\text{m}$ amplitude fluctuations), we performed an additional experiment to test this and to provide validation of the precision of the estimated motion parameters by showing that their fluctuations correspond to real subject motion, even at very high resolution. For this experiment, we needed a shorter $\text{TR}_{\text{volume}}$ to be able to reliably sample the respiration cycle, so we used a 3D FatNav with 4 mm resolution and $4 \times 4 = 16$ acceleration, resulting in $\text{TR}_{\text{volume}} = 230$ ms. Experiments 2 and 3 used a sampling rate for the FatNavs of 6 and 2 s, respectively (the TR of the respective sequences), which is also too long to reliably sample the respiratory cycle. Typical respiration cycles, however, should be adequately sampled by a volume TR of 230 ms.

A scan consisting only of 450 3D FatNavs was acquired, covering ~ 2 min with simultaneous logging of the data from the respiratory belt supplied with a scanner for physiological monitoring. Processing to obtain motion estimates from the FatNavs was identical to the previous experiments. For easier visual comparison of the respiratory trace with the z-component of the motion estimates, the estimated z-motion values were high-pass filtered to remove low-frequency drifts.

RESULTS

Experiment 1: Evaluation of Achievable GRAPPA Acceleration for 3D FatNavs

Figure 2 compares reconstructions of a single slice out of a fully sampled 3D-GRE acquisition after retrospective decimation to simulate acquisitions at increasing two-dimensional acceleration factors, following reconstruction using GRAPPA. The reconstructions from nonselective excitation data (Fig. 2a) exhibited small but noticeable artifacts at 4×4 acceleration, which became very strong when the acceleration reached 6×6 . For the reconstructions from the fat excitation data, there was only very minor deterioration of image quality up to acceleration of $6 \times 6 = 36$, but at $10 \times 10 = 100$ the edges started to become less well-defined, and increased noise

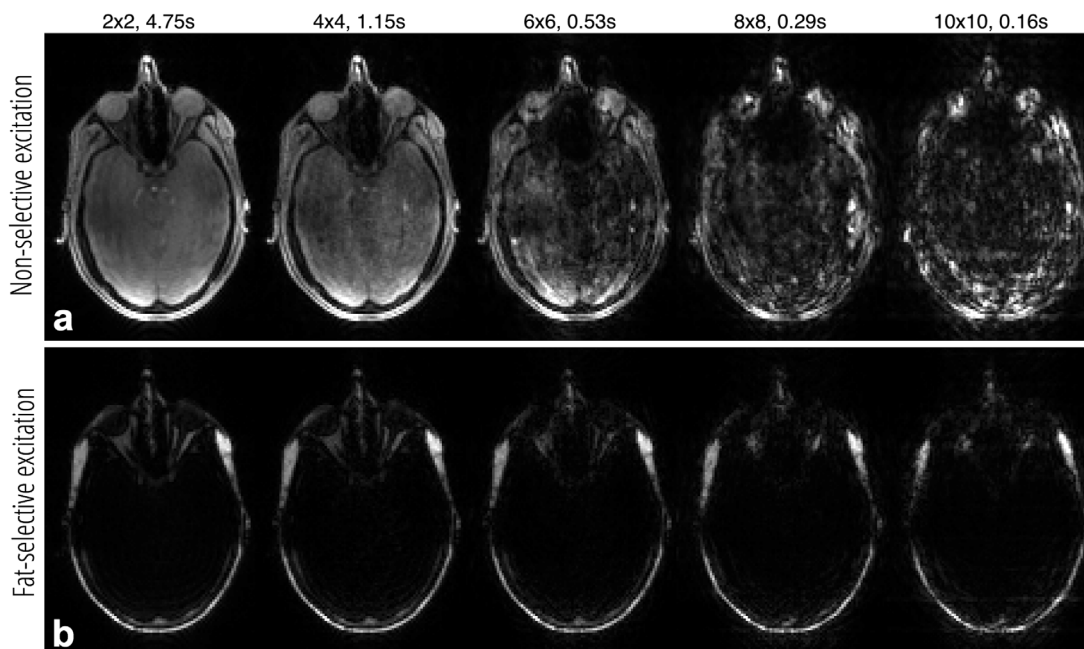


FIG. 2. A single slice of a 3D GRE acquisition of the whole head using (a) nonselective excitation and (b) fat excitation. The data were retrospectively undersampled by increasing acceleration factors (2×2 through to 10×10 , with corresponding TR_{volume} also shown) and reconstructed using GRAPPA weights determined from separate calibration data.

and artifacts were visible. Even at the highest acceleration factor, however, the outline of the scalp remained recognizable.

Experiment 2: High-Resolution MP2RAGE Scan Motion-Corrected with 3D FatNavs

Figure 3a shows the rigid body motion parameters estimated from the 3D FatNavs (2 mm, 4×4 acceleration) during the ~ 37 -min MP2RAGE scan. All plots pass through zero at ~ 12 min, as this corresponds to the time of the acquisition of the center of k-space, and motion parameters were defined relative to this head pose. The amplitude of the estimated motion was small, with a root-mean-square (RMS) displacement of 1.08 mm and RMS rotation of 0.84° during the ~ 37 -min scan.

Figures 3b and 3c compare the MP2RAGE contrast before and after motion correction. When viewed at this scale, the differences are nearly imperceptible. However, as illustrated by the difference image (Fig. 3d), differences between the two are primarily high-resolution features.

The zoom of the MP2RAGE contrast shown in Figure 4 demonstrates visible improvements in image quality following motion correction. This is mostly visible by comparing features with high spatial frequency information, such as arteries (bright), veins (dark in the white matter toward the right of the image), and between the ventricles. Such high-resolution differences are confirmed by the difference image. Differences also become more obvious to the eye when the images are alternated as a movie (Supporting Video S1).

It was found that visualizations of the blood vessels increase the visual perceptibility of the improvements in image quality following motion correction. Figure 5

shows the minimum intensity projection over a 10-mm-thick slab in the z-direction of a zoomed section of part of the GRE_{T12} volume from the same MP2RAGE dataset. Visual inspection revealed noticeable improvements in vessel sharpness following motion correction, especially in the conspicuity of the smaller veins within the white matter and deep brain (Supporting Video S2 shows the same image comparison).

Figure 6 shows a maximum intensity projection over the full 80-mm slab in the z-direction of the same GRE_{T12} volume, visualizing the arteries. Again, the main difference following motion correction was an increased conspicuity of the smaller vessels (Supporting Video S3 shows the same image comparison).

Experiment 3: High-Resolution TSE Scan Motion-Corrected with 3D FatNavs

Figure 7a shows the estimated rigid body motion parameters from the 3D FatNavs (2 mm, 4×4 acceleration) during the ~ 34 -min TSE scan. The total motion for this subject was very small, with an RMS displacement of 0.40 mm and RMS rotation of 0.18° . All motion parameters passed through zero at around 17 min, as all parameters had been shifted to coincide with the acquisition of the center of k-space.

Figures 7b and 7c compare orthogonal views of the whole high-resolution TSE dataset, before and after the application of retrospective motion correction. While overall the images appear comparable, the difference image demonstrates that the major changes are high-spatial frequencies (ie, edges) (Fig. 7d).

When examining a zoomed sagittal view of the anterior of the brain from the same TSE dataset, clear improvements in delineation of image boundaries were observed,

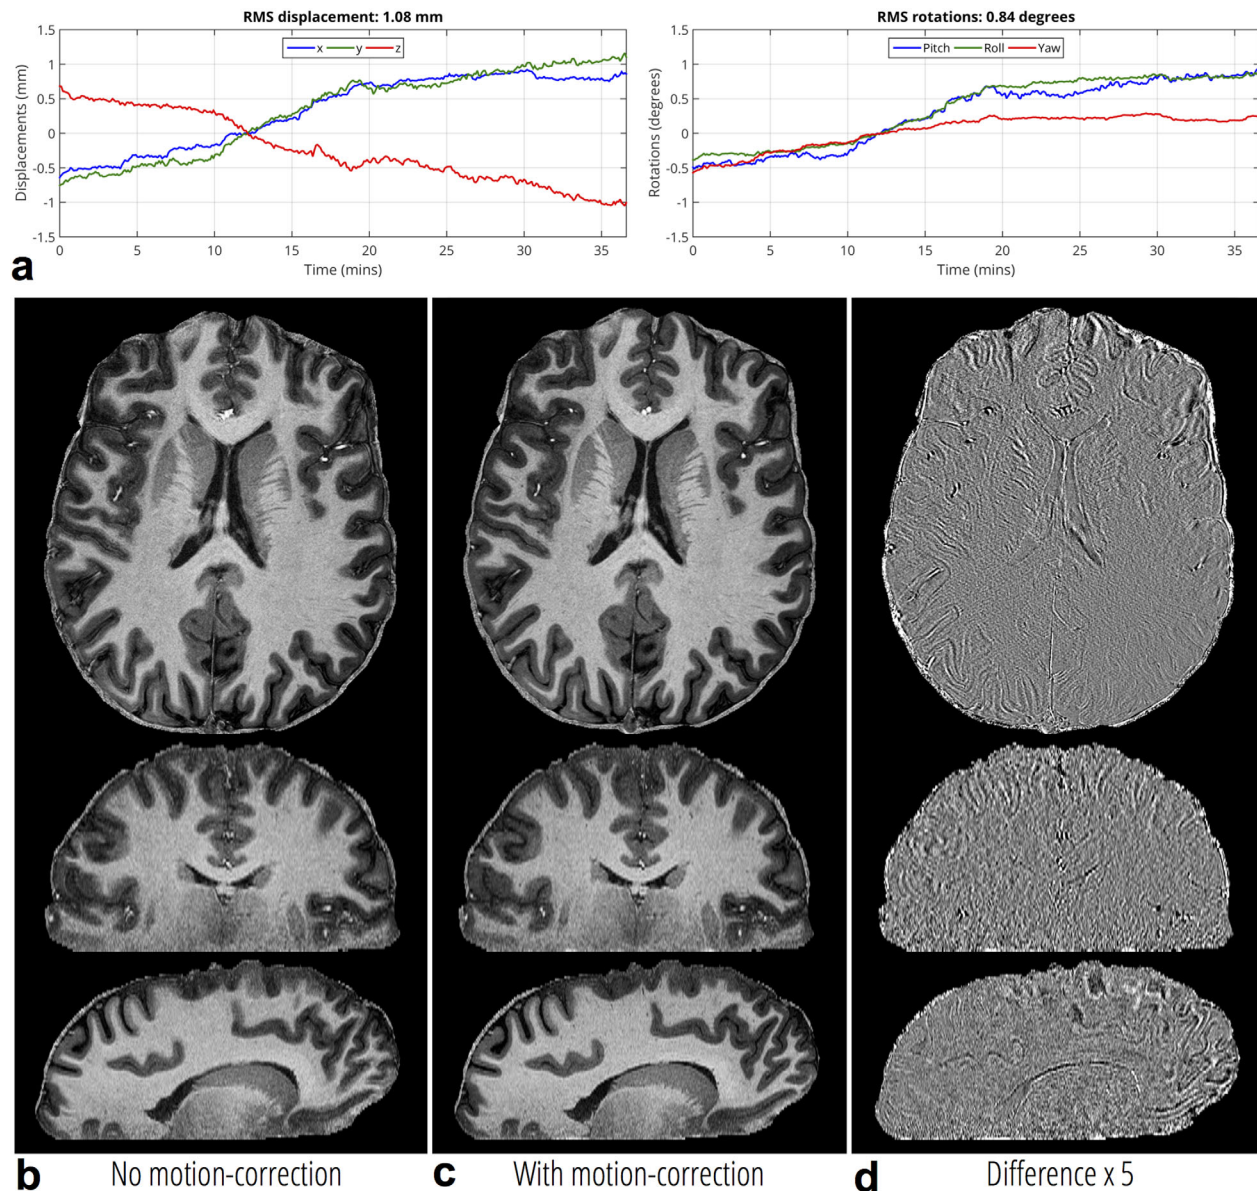


FIG. 3. a: Estimated rigid body motion parameters obtained from 3D FatNavs (isotropic resolution, 2 mm; acceleration, 4×4) during the ~ 37 -min MP2RAGE scan (resolution, $0.33 \times 0.33 \times 1.00$ mm) (Experiment 2). b: The high-resolution MP2RAGE volume. c: The same MP2RAGE volume following retrospective motion correction based on the estimated motion from the FatNavs. d: The difference between the images before and after motion correction.

especially at the boundary between the very bright cerebrospinal fluid and the gray matter (Fig. 8). Ringing artifacts across the cortex resulting from the bright cerebrospinal fluid were also noticeably reduced after motion correction. Larger arteries, which appeared dark in these images, were also more clearly identifiable (Supporting Video S4 shows an animated version of this figure).

Experiment 4: Detection of Head Motion Due to the Respiratory Cycle with 3D FatNavs

Figure 9 shows the estimated motion parameters from the 2-min scan consisting only of 3D FatNavs (4 mm, 4×4 acceleration). Visual comparison shows that data

from the respiratory belt explain much of the fluctuations observed in the estimated z-motion (Fig. 9c).

DISCUSSION

Retrospective Motion Correction

An advantage of the retrospective correction over prospective correction is that the uncorrected image is always also available. Even in the current proof-of-concept implementation with prolonged off-line processing of raw data, the original uncorrected images appear on the scanner via the standard reconstruction pipeline. In order for the method to be as robust as possible, it may be useful to devise an automated quality check of the corrected image to alert the user that they may wish

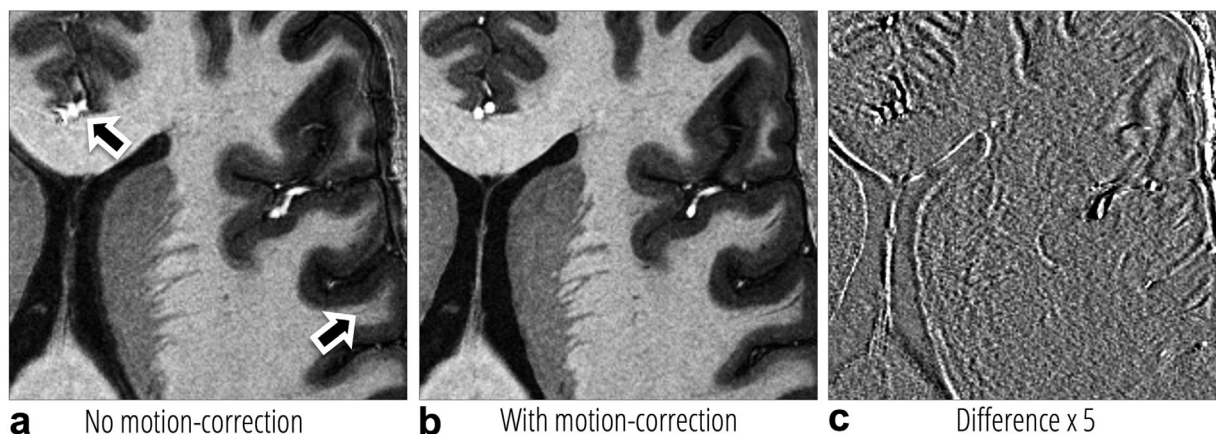


FIG. 4. a: Magnified image of the MP2RAGE dataset shown in Figure 3. Arrows indicate regions where the improvement is most prominent. b: The same section following retrospective motion correction. c: The difference between the two images. The overall improvement can be seen more clearly in Supporting Video S1.

to refer back to the original uncorrected images in the case of an anomaly in the retrospective pipeline.

In its current implementation, the retrospective motion correction is limited to 3D sequences without parallel acceleration. Incorporation of support for parallel acceleration of the host sequence would require a reconstruction approach that is capable of dealing with k -space data that no longer conforms to a Cartesian grid, such as non-Cartesian SENSE (23). As this would present additional complications to implement robustly in 3D at high resolution, the results we present here were all acquired without parallel acceleration.

In principle, the 3D FatNav approach can also be used for prospective motion correction, provided that real-time image reconstruction pipelines available on the scanner software/hardware and the available memory are capable of coping with the demands of highly accelerated GRAPPA (the computational load and memory burden both increase with increasing acceleration factor). A more optimized approach to the image reconstruction would likely be required, both in terms of memory demands and processor load, to reduce the latencies to an acceptable level for prospective motion correction.

The image coregistration also represents a significant computational burden that would need to be optimized in this case.

3D FatNav Reconstruction and Coregistration

For the chosen parameters of the 3D FatNavs (2 mm, 4×4) used to estimate motion parameters for the structural scans, we observed a high precision of motion estimates on the order of approximately $<25 \mu\text{m}$ and approximately $<0.025^\circ$ (the estimated amplitude of the high-frequency fluctuations visible in Figs. 3a and 7a), but we do not have an independent measure of the remaining bias in these estimates. It is reassuring that the images from the host sequence following motion correction are visibly improved in terms of image sharpness, especially in the increased conspicuity of very small vessels. The current choices of resolution and acceleration for the 3D FatNavs are somewhat arbitrary, and further investigation will be necessary to determine the optimal parameters for a given dead time available in a particular host sequence. This optimization, however, will inevitably also depend on both the choice of parallel imaging

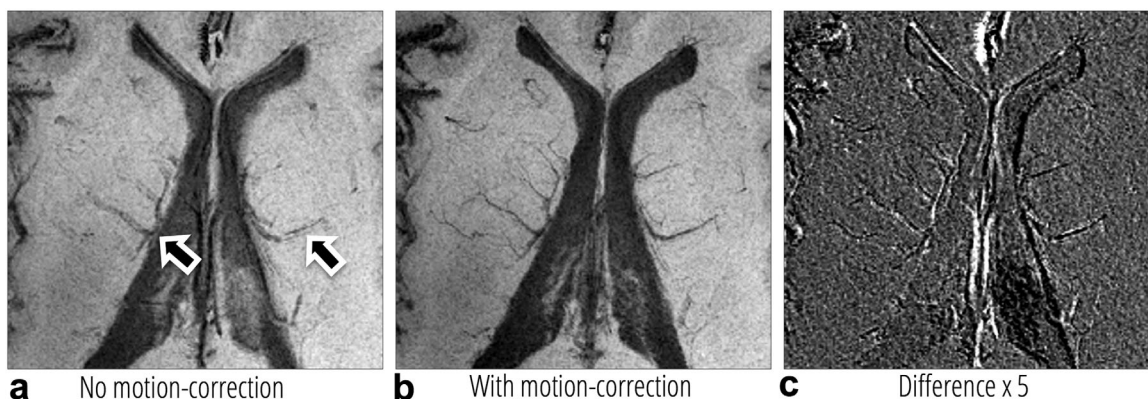


FIG. 5. a: Magnified image of the GRE_{T12} volume from the MP2RAGE dataset shown in Figures 3 and 4, with a minimum intensity projection taken over a 10-mm slab in the z -direction. Arrows indicate regions where the improvement is most prominent. b: The same section following retrospective motion correction. c: The difference between the two images. The overall improvement can be seen more clearly in Supporting Video S2.

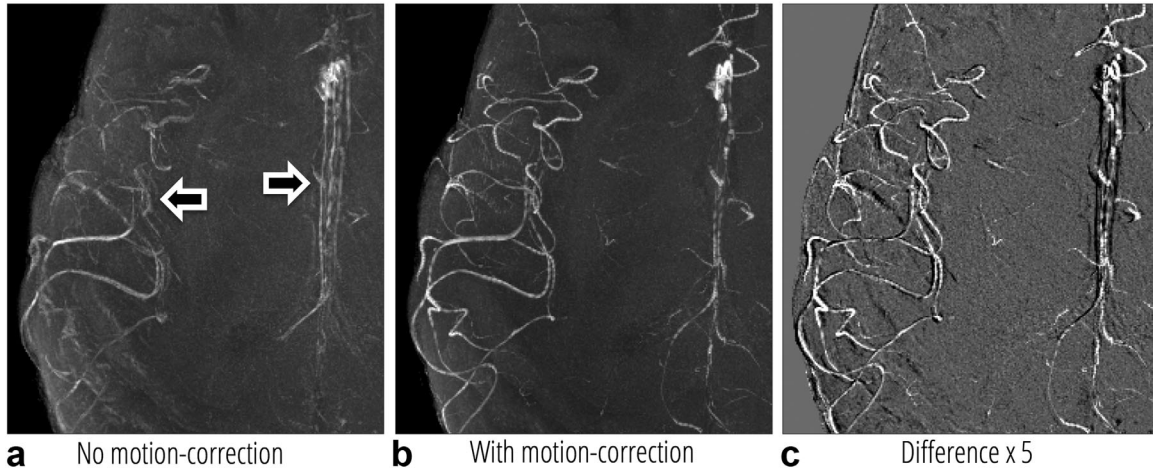


FIG. 6. a: Magnified image of the GRE_{T12} volume from the MP2RAGE dataset shown in Figures 3–5, with a maximum intensity projection taken over the full 80-mm slab in the z-direction. Arrows indicate regions where the improvement is most prominent. b: The same section following retrospective motion correction. c: The difference between the two images. The overall improvement can be seen more clearly in Supporting Video S3.

reconstruction method and the image registration parameters.

The results from Experiment 4 suggest that the even the lower-resolution 3D FatNavs (4 mm, 4×4) are sufficiently sensitive to track the small motion associated with the respiratory cycle; however, in order to usefully correct for this motion, it becomes important to be able to usefully estimate the position in the respiratory cycle corresponding to when the host sequence data were acquired, rather than at the time of the navigator. As can be observed from Figure 1, the timing of the MP2RAGE and TSE sequences is such that the chosen navigator used for those experiments would be too long to be able to correct respiratory-induced movements. The quality of our preliminary results of motion correction with FatNavs (where we do not expect to have corrected for respiratory-induced motion) suggests that correcting for the slow drifting movements over the entire scan duration is more critical to image quality than the faster oscillations due to the respiratory cycle. Further investigation is necessary to determine in which situations accurate correction of respiratory-induced motion might provide additional noticeable improvement in image quality.

Given that the fat signal is primarily localized to the tissue surrounding the skull, it is expected that there will be fewer identifiable structural features than in a typical brain image, which may impair convergence of the coregistration, especially in the case of rotations where the subject has a round head shape. Our experience in a limited number of subjects is that the precision of motion estimates is not prohibitively hindered by this effect, presumably as clear features such as the temporal muscle and the ocular fat surrounding the eyes (both visible in Fig. 2b) are able to help yield robust coregistration. This assumption will need to be revisited after a greater number of subjects have been scanned.

In Experiment 3, there was noticeably more noise in the estimated z-displacement compared with the x and y

displacements (Fig. 7a), an effect not observed in Experiment 2 (Fig. 3a). This is likely due to the difference in the respiration-induced motion between volunteers.

The coregistration of the 3D FatNavs was performed with SPM's realign tool, using the least-squares difference as the cost function. This could potentially lead to biased motion estimates, especially if aliasing artifacts are present as a result of the high acceleration factors used. We expect that it could be beneficial to exploit the fact that a full 3D image of the fat is generated from the GRAPPA calibration data acquired at the start of the acquisition. Each individual 3D FatNav is, to a first approximation, exactly the same image following some small rigid body motion. Incorporating the prior knowledge of the object should allow improved reconstruction of each FatNav—and thus more robust estimates of head motion.

We currently acquire the calibration data for the GRAPPA weights for the 3D FatNavs only once at the start of the scan (2.3 s). If the subject motion is large, it may be beneficial to update the GRAPPA weights during the scan. This could be achieved without additional scan time if the k-space points acquired for each FatNav are shifted relative to the previous FatNav. As a consequence, for every 16 FatNavs acquired, a full coverage of k-space can be achieved (using 16-fold acceleration). It would also be possible in this way to have a “sliding window” of GRAPPA weights for the reconstruction of each individual FatNav to try to make the reconstruction more robust to aliasing artifacts by always having a set of GRAPPA weights from a head pose as close as possible to the head pose at the time of the FatNav. We primarily envisage early applications of the technique to remain with the correction of small involuntary motion of compliant subjects, however, as not only is larger motion more difficult to track accurately, but it will also lead to larger gaps in the corrected k-space of the host sequence, which can also lead to artifacts.

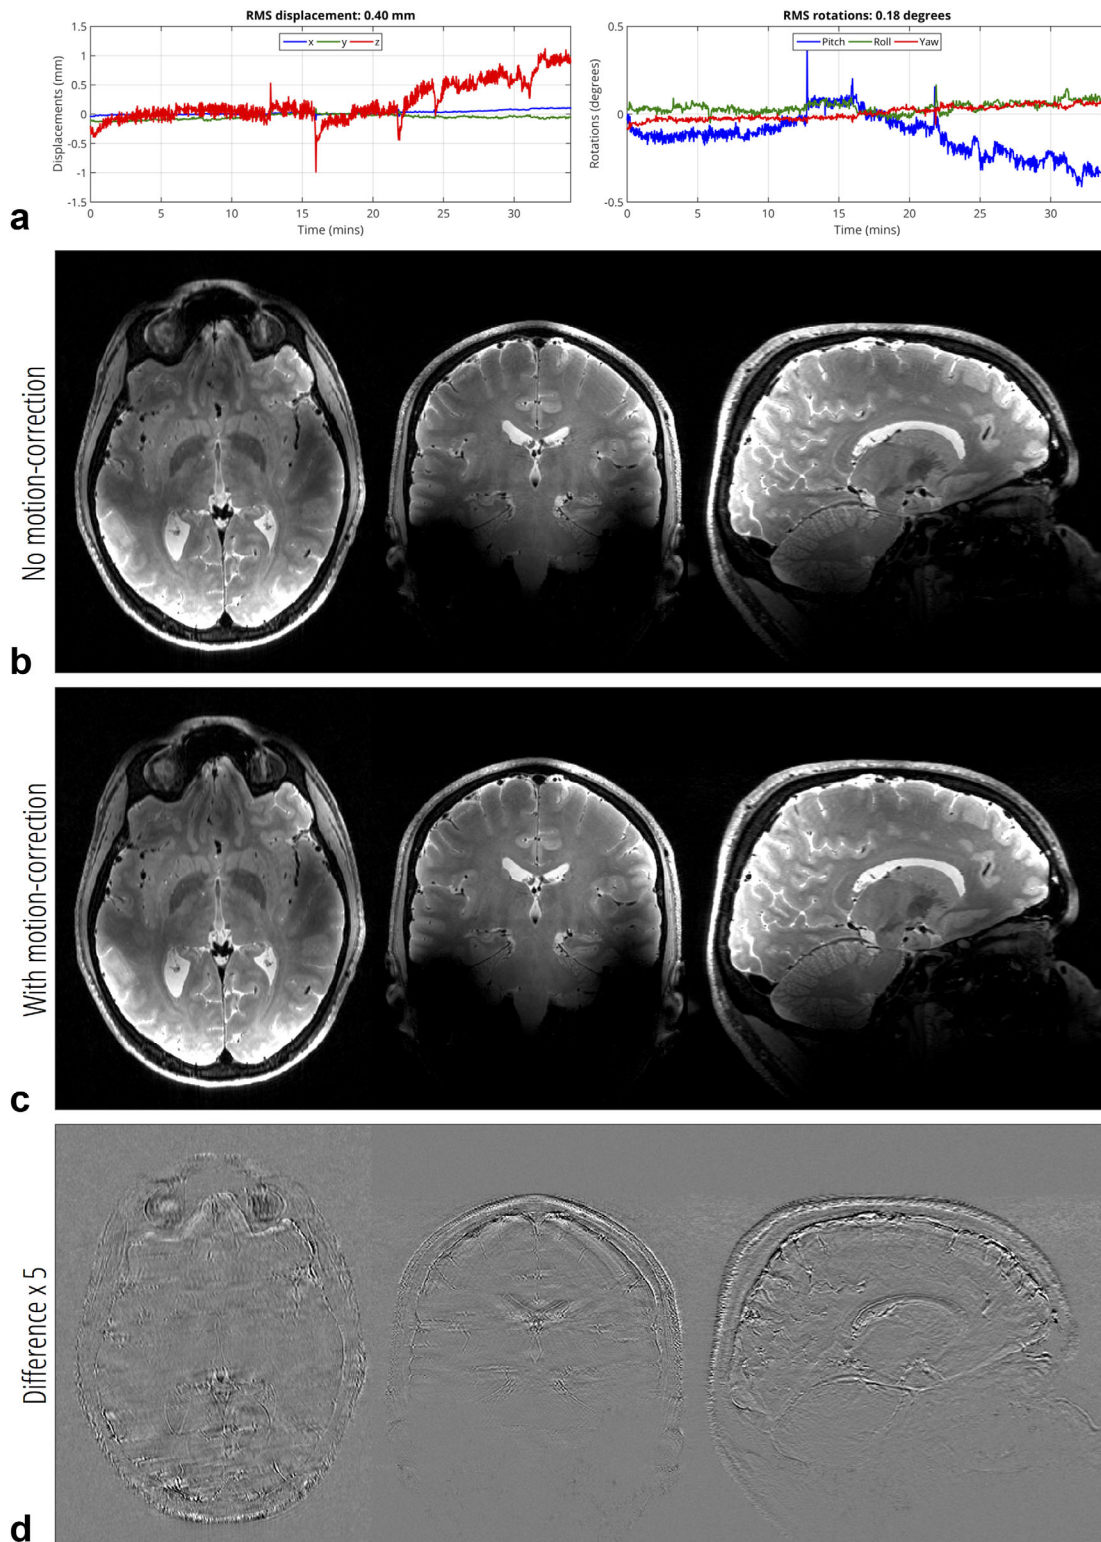


FIG. 7. a: Estimated rigid body motion parameters obtained from 3D FatNavs (isotropic resolution, 2 mm; acceleration, 4×4) during the ~ 34 -min TSE scan (isotropic resolution, $600 \mu\text{m}$) (Experiment 3). b: High-resolution TSE volume. c: The same TSE volume following retrospective motion correction. d: The difference between the two images.

3D FatNavs at Other Field Strengths

Although the present study was conducted at 7T, the 3D FatNav is expected to be applied easily at lower fields.

Although the duration of the binomial fat excitation will be longer due to the smaller frequency shift between fat and water resonances, this should not lead to prohibitively long scan times for the 3D FatNav.

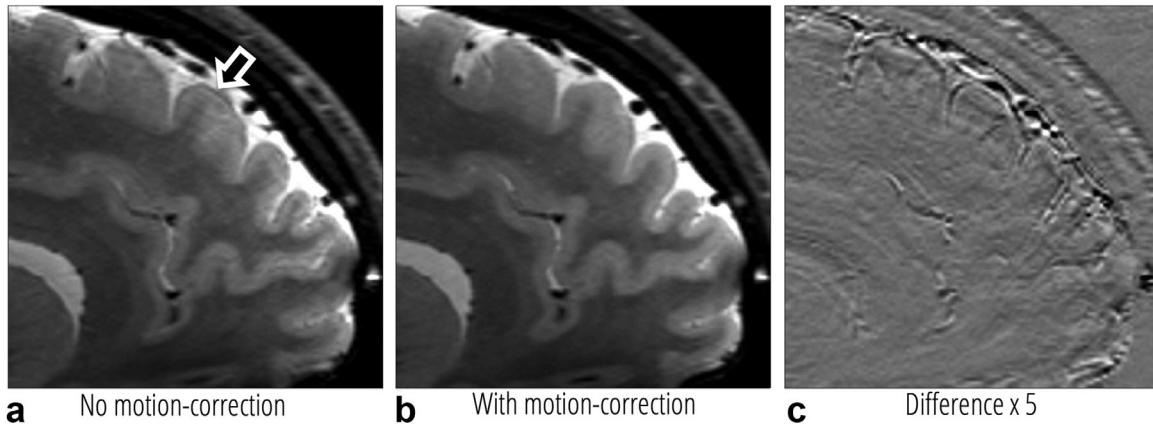


FIG. 8. a: Magnified sagittal view of the TSE dataset shown in Figure 7. Arrows indicate regions where the improvement is most prominent. b: The same image following retrospective motion correction. c: The difference between the two images. The overall improvement can be seen more clearly in Supporting Video S4.

3D FatNavs in Other Host Sequences

We demonstrated the insertion of 3D FatNavs into an MP2RAGE and a TSE sequence, as these are both commonly used protocols which already have sufficient dead time to allow insertion of the navigator with no penalty in scan time. It would also be desirable to be able to apply motion correction to sequences such as high-resolution GRE for susceptibility-weighted imaging, but this will inevitably require a longer scan duration to incorporate the 3D FatNavs. There is therefore considerable interest in capturing high-resolution motion infor-

mation in as short a navigator as possible. The remarkably high quality of the fat images presented in Figure 2 at exceptionally high acceleration factors might give the impression that acquisitions as short as 290 ms (8×8 acceleration) may still yield high-quality motion estimates. However, our preliminary results attempting to assess the increasing error and bias associated with increasing acceleration factor suggest that, at least with the current image registration pipeline, the (visually) small artifacts associated with the high acceleration factors can introduce unacceptable levels of bias in the

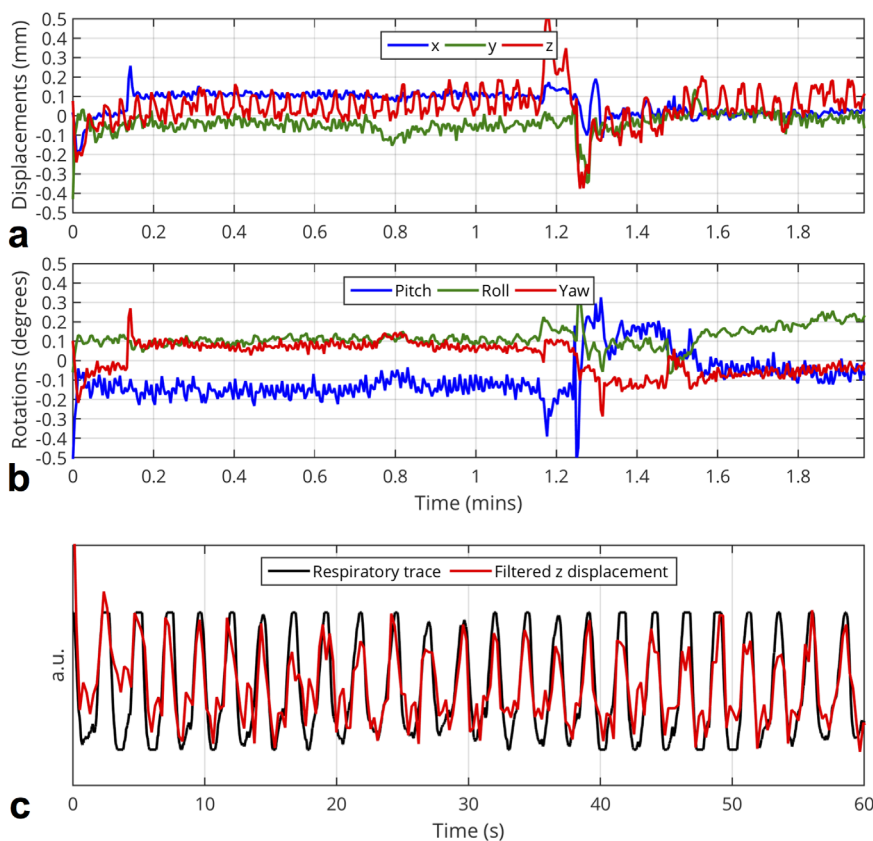


FIG. 9. a, b: Estimated motion parameters from a 2-min scan consisting only of 3D FatNavs, with resulting translations (a) and rotations (b). c: Magnification of the first 60 s of the estimated z-displacement (after high-pass filtering) shown on the same axes as the signal measured from a respiratory belt.

motion estimates (24). Future work will investigate whether incorporating prior knowledge regarding the structure of these artifacts can improve motion estimates from customized image registration algorithms for very fast FatNav acquisitions. In addition to the increased scan duration, care will also need to be taken to ensure that FatNavs can be inserted without significantly disturbing the steady-state properties of the GRE host sequence, as has been successfully achieved for the EPI-based vNavs (25).

CONCLUSION

We have successfully demonstrated the feasibility of highly accelerated fat excitation volumes to be used as motion navigators for the retrospective correction of microscopic involuntary movement of compliant subjects during high-resolution 3D structural scans of extended duration, yielding noticeable improvements in image quality even for very small motion of the subject.

REFERENCES

- Zaitsev M, Dold C, Sakas G, Hennig J, Speck O. Magnetic resonance imaging of freely moving objects: prospective real-time motion correction using an external optical motion tracking system. *Neuroimage* 2006;31:1038–1050.
- Ooi MB, Krueger S, Thomas WJ, Swaminathan SV, Brown TR. Prospective real-time correction for arbitrary head motion using active markers. *Magn Reson Med* 2009;62:943–954.
- Schulz J, Siegert T, Reimer E, Labadie C, Maclaren J, Herbst M, Zaitsev M, Turner R. An embedded optical tracking system for motion-corrected magnetic resonance imaging at 7T. *Magn Reson Mater Phy* 2012;25:443–453.
- Qin L, van Gelderen P, Derbyshire JA, Jin F, Lee J, de Zwart JA, Tao Y, Duyn JH. Prospective head-movement correction for high-resolution MRI using an in-bore optical tracking system. *Magn Reson Med* 2009;62:924–934.
- Maclaren J, #Armstrong BSR, Barrows RT, et al. Measurement and correction of microscopic head motion during magnetic resonance imaging of the brain. *PLoS One* 2012;7:e48088.
- Pipe JG. Motion correction with PROPELLER MRI: application to head motion and free-breathing cardiac imaging. *Magn Reson Med* 1999;42:963–969.
- Anderson AG, Velikina J, Block W, Wieben O, Samsonov A. Adaptive retrospective correction of motion artifacts in cranial MRI with multi-coil three-dimensional radial acquisitions. *Magn Reson Med* 2013;69:1094–1103.
- White N, Roddey C, Shankaranarayanan A, Han E, Rettmann D, Santos J, Kuperman J, Dale A. PROMO: real-time prospective motion correction in MRI using image-based tracking. *Magn Reson Med* 2010;63:91–105.
- Van der Kouwe AJW, Benner T, Dale AM. Real-time rigid body motion correction and shimming using cloverleaf navigators. *Magn Reson Med* 2006;56:1019–1032.
- Welch E, Manduca A. Spherical navigator echoes for full 3D rigid body motion measurement in MRI. *Magn Reson Med* 2001;41:32–41.
- Tisdall MD, Hess AT, Reuter M, Meintjes EM, Fischl B, van der Kouwe AJW. Volumetric navigators for prospective motion correction and selective reacquisition in neuroanatomical MRI. *Magn Reson Med* 2012;68:389–399.
- Schulze P, Stucht D, Danishad KA, Kadashevich IY, Herbst M, Lovell-smith C, Maclaren J, Barrows RT, Kusik TP. Prospective Motion Correction to Increase the Achievable Resolution in Brain Imaging at 7T. In Proceedings of the 20th Annual Meeting of ISMRM, Melbourne, Victoria, Australia, 2012. p. 597.
- Tisdall MD, Polimeni JR, van der Kouwe AJW. Motion-Corrected 350 μm Isotropic MPRAGE at 3T Using Volumetric Navigators (vNavs). In Proceedings of the 21st Annual Meeting of ISMRM, Salt Lake City, Utah, USA, 2013. p. 268.
- Nguyen TD, Nuval A, Mulukutla S, Wang Y. Direct monitoring of coronary artery motion with cardiac fat navigator echoes. *Magn Reson Med* 2003;50:235–241.
- Van der Kouwe AJW, Benner T, Wald LL. Decoupling motion navigation from imaging using spatial-spectral RF pulses. In Proceedings of the 16th Annual Meeting of ISMRM, Toronto, Ontario, Canada, 2008. p. 1465.
- Skare S, Hartwig A, Mårtensson M, Avventi E, Engström M. Properties of a 2D fat navigator for prospective image domain correction of nodding motion in brain MRI. *Magn Reson Med* 2015;73:1110–1119.
- Griswold MA, Jakob PM, Heidemann RM, Nittka M, Jellus V, Wang J, Kiefer B, Haase A. Generalized autocalibrating partially parallel acquisitions (GRAPPA). *Magn Reson Med* 2002;47:1202–1210.
- Marques JP, Kober T, Krueger G, van der Zwaag W, Van de Moortele P-F, Gruetter R. MP2RAGE, a self bias-field corrected sequence for improved segmentation and T1-mapping at high field. *Neuroimage* 2010;49:1271–1281.
- Fessler J, Sutton B. Nonuniform fast Fourier transforms using min-max interpolation. *IEEE Trans Signal Process* 2003;51:560–574.
- Van de Moortele P-F, Auerbach EJ, Olman C, Yacoub E, Uğurbil K, Moeller S. T1 weighted brain images at 7 Tesla unbiased for Proton Density, T2* contrast and RF coil receive B1 sensitivity with simultaneous vessel visualization. *Neuroimage* 2009;46:432–446.
- Zhang Y, Brady M, Smith S. Segmentation of brain MR images through a hidden Markov random field model and the expectation-maximization algorithm. *IEEE Trans Med. Imaging* 2001;20:45–57.
- Mugler J, Kiefer B, Brookeman J. Three-Dimensional T2-Weighted Imaging of the Brain Using Very Long Spin-Echo Trains. In Proceedings of the 8th Annual Meeting of ISMRM, Denver, Colorado, USA, 2000. p. 687.
- Pruessmann KP, Weiger M, Börner P, Boesiger P. Advances in sensitivity encoding with arbitrary k-space trajectories. *Magn Reson Med* 2001;46:638–651.
- Gallichan D, Marques JP, Gruetter R. Optimizing a highly-accelerated FatNav for high-resolution motion-correction. In Proceedings of the 23rd Annual Meeting of ISMRM, Toronto, Ontario, Canada, 2015 Abstract #2481.
- Tisdall MD, Bhat H, Heberlein K, van der Kouwe AJW. Prospective head motion correction in 3D FLASH using EPI-based volumetric navigators (vNavs). In Proceedings of the 22nd Annual Meeting of ISMRM, Milan, Italy, 2014. p. 882.

SUPPORTING INFORMATION

Additional Supporting Information may be found in the online version of this article.

Video S1. Animated version of Figure 4. A zoomed section of the MP2RAGE volume from Experiment 2, showing the improvements following retrospective motion correction using the 3D FatNavs.

Video S2. Animated version of Figure 5. A zoomed section of the GRE_{T12} volume from the MP2RAGE dataset from Experiment 2, with a minimum intensity projection taken over a 10 mm slab in the z-direction, showing the improvements following retrospective motion correction using the 3D FatNavs.

Video S3. Animated version of Figure 6. A zoomed section of the GRE_{T12} volume from the MP2RAGE dataset from Experiment 2, with a maximum intensity projection taken over the full 80-mm slab in the z-direction, showing the improvements following retrospective motion correction using the 3D FatNavs.

Video S4. Animated version of Figure 8. A zoomed section of the TSE volume from Experiment 3, showing the improvement following retrospective motion correction using the 3D FatNavs.